



# ROLYAN SPLINT BATH USER MANUAL

---

REF 100.500 Standard Size

REF 100.501 Large Size

This manual must be given to the user of the product. Before using this product, this manual must be read and saved for future reference.

---



Manufactured by:  
**STRAVA SOLUTIONS**  
2733 Kanasita Drive #125  
Hixson, TN 37343 USA



# CONTENTS

---

Inspection	3
Contents of Box	3
Safety	3
Symbols	4
The Purpose of this Manual	6
Instructions for Proper Use	6
Indications for Use	6
Product Description	7
Technical Data	8
Material	9
Responsibility of the User	9
Instructions	10
Initial Set Up	10
Troubleshooting	14
Replacement Parts	14
Warranty/Replacements	15
Service Life	15
Storage and Handling	15
Product Labeling	16

# ROLYAN SPLINT BATH USER MANUAL

---

## Inspection

Prior to shipment, the water baths are subjected to a thorough safety-related and functional quality control and are carefully packed.

Check **ALL** parts for shipping damage. If shipping damage is noted, **DO NOT USE**. Contact dealer/manufacturer for further instruction.


Products may only be returned in undamaged cardboard packaging – primarily the original cardboard packaging..

## Contents of Box

1. Splint Bath – Standard REF 100.500 or Large REF 100.501
2. User Manual REF 400.500
3. US Hospital Grade Power Cord REF 300.107
4. 8 ft Drain Hose REF 200.101

## Safety

The safety section contains important information for the safe operation and use of this product. Read this information and any other safety information included with the product before using the splint bath.

	<b>WARNING</b> To avoid electric shock, connect the instrument to properly earth-grounded, GFCI protected, 3-prong receptacles only. Failure to observe this precaution can result in severe injury.
---	---

The Electric Shock Symbol is used to indicate a hazard arising from dangerous voltage. Any mishandling could result in severe injury or death. The Exclamation Symbol appears in Warning and Caution statements.



This symbol designates where personal injury or damage to the equipment is possible.

# SYMBOLS

---

Signal words are used in this manual and apply to hazards or unsafe practices which could result in personal injury or property damage. See the information below for definitions of the signal words.



**DANGER!**

## **DANGER!**

Danger indicates an imminently hazardous situation which, if not avoided, will result in death or serious injury.



**WARNING!**

## **WARNING!**

Warning indicates a potentially hazardous situation which, if not avoided, could result in death or serious injury.

- *Failure to follow these instructions could result in damage to your new heating appliance and/or injury*












**CAUTION!**

## **CAUTION!**

Caution indicates a potentially hazardous situation which, if not avoided, may result in property damage or minor injury or both.



SYMBOL	DESCRIPTION
	European Union CE mark. The CE mark indicates that this product satisfies the relevant requirements of EC Directives.
	Authorized representative in the European Community
	Waste Electrical and Electronic Equipment (WEEE) This symbol on the product or on its packaging indicates that this product must not be disposed of with regular waste. Instead, it is the user's responsibility to dispose of waste equipment according to the local laws. Separate collection and recycling of the waste equipment at the time of disposal will help conserve natural resources and ensure it is recycled in a manner that protects human health and the environment. For information about where the user can drop off the waste equipment for recycling, please contact your local waste collection authority.
	Electric Shock The Electric Shock Symbol is used to indicate a hazard arising from dangerous voltage. Any mishandling could result in severe injury or death.
	Caution, consult the instructions for use.
	Keep dry
	Refer to User Manual
SGS inspection mark	Product Certification Mark
	Year of Manufacture
	Catalogue Number

# THE PURPOSE OF THIS MANUAL

---

This User Manual is mainly focused on the set up, cleaning, operation and routine maintenance of the Rolyan Splint Bath. These instructions help avoid dangers and repairs while increasing product reliability. Keep this manual for future reference.

## Instructions for Proper Use



Please read these instructions carefully before using the water baths.

These instructions will help avoid dangers, unnecessary repair costs and down times. Following these instructions will increase the reliability and life of the product.

The water bath is only intended for the heating of thermoplastic material for medical use.



- This water bath is not suitable for direct heating without using water.
- The heating of food and drinks, as well as other pharmaceutical and medical products, is not allowed and constitutes improper use.
- Direct application on the patient is not allowed.

## Indications for Use

The Rolyan Splint Bath is intended for use as a reservoir in hospitals, clinics and other medical facilities to heat and soften thermoplastic used in the splinting process. The device is intended for indoor use only.

---

## Product Description

Rolyan Splint Bath is a reservoir made of a thermoset composite material that holds and heats water. The water bath allows for thermoplastic splint sheets to be softened and made pliable to form to the body. The Rolyan Splint Bath has a custom LCD display for accurate water temperature readings, user-controlled water temperature and time settings, thermoplastic sheet presets, user presets, sanitation cycles and automatic water drainage. The Rolyan Splint Bath is equipped with three (3) models of cleaning: continuous UV light, a sanitation cycle that heats the water temperature to kill levels, and quick water evacuation. The Rolyan splint bath has a transparent, fold-up glass lid, a thermostat water temperature regulator (+/-2F), and holds approximately 5.2 gallons of water.



# TECHNICAL DATA

## Technical Specifications Rolyan Splint Bath

ROLYAN SPLINT BATH STD	UM	Spec
REF 100.500		
Operating Temperature Range	F	140° - 185° F
	C	60° - 85° C
Temperature Variability	F	5°
	C	
Power Consumption	W	1500 W
Frequency	Hz	50/60 Hz
Mains Voltage	V	100-230 VAC
AC Current	A	<13 Amps
Water Fill Capacity	Gallons	5.2 G
	Litres	20 L
Water Fill Height	in	5"
	cm	12.5 cm
Unit Weight	lbs	35 lbs
	kg	15.9 kg
Unit Dims (LxHxW)	in	23.5"L 20.5"W 10"H
	cm	60cm L 52cm W 25.5cm H
Standard		IEC 61010-1, -2
		UL 61010-1, -2
		CSA C22.2#61010-1, -2
		CB SCHEME

ROLYAN SPLINT BATH LG	UM	Spec
REF 100.501		
Operating Temperature Range	F	
	C	
Temperature Variability	F	
	C	
Power Consumption	W	1500 W
Frequency	Hz	50/60 Hz
Mains Voltage	V	100-230 VAC
AC Current	A	<13 Amps
Water Fill Capacity	Gallons	
	Litres	
Water Fill Height	in	
	cm	
Unit Weight	lbs	
	kg	
Unit Dims (LxHxW)	in	
	cm	
Standard		IEC 61010-1, -2
		UL 61010-1, -2
		CSA C22.2#61010-1, -2
		CB SCHEME



## Material

The outer chassis material is a thermoset composite material. The unit consists of a tempered glass lid, drainage hose, water strainer, water pump, power supply and ultraviolet (UV) light.

## Responsibility of the User

This product guarantees safe operation if installed, operated and maintained in accordance with general safety rules. The operator of this device must read and understand this manual and be trained in occupational therapy methods. All operators are to be aware of the relevant dangers of using a hot water bath and exercise measures to avert such dangers.

## Control Panel

- 1 - Target temperature display
- 2 - Actual temperature display
- 3 - Temperature display mode °C/°F
- 4 - Time control up or down
- 5 - Timer START/STOP button
- 6 - Timer - time count down display
- 7 - Presets wheel
- 8 - Real time display
- 9 - Menu
- 10 - Add a new preset
- 11 - Power down unit



Side of Unit



Rear of Unit



Top Side of Unit



# INSTRUCTIONS



WARNING: Do not start the unit if the cable or plug is damaged, if there are obvious, visible defects to the unit, or if the drain valve is not adequately closed.

## Initial Set Up


- Unpack the splint bath and place on a level surface that is capable of bearing the bath and water load. Be sure there is adequate space between the vent and wall for ventilation.
- Make sure that the unit is unplugged, and all packaging materials are cleared from the reservoir.
- Fill the unit with water approximately 5 inches deep and close the hinged lid. Be sure that the power is off when filling the tank with water.
- Locate the power switch at the back of the unit and turn the unit “on”.
- At initial powering up of the bath, the start up wizard will display on the LCD screen.
  - Start up wizard will prompt user to set time, day of the week, and temperature.
  - **Note:** Sanitation cycle defaults to “on”.

## Control panel:

The touchscreen LCD display lights up when the unit is turned on. The control panel functionality provides the user with options to customize the device for their needs.

- The home screen consists of the session time, current water temperature, set temperature, presets, real time, and a menu icon.
- Presets are factory installed temperature and time suggestions that are specific to the thermoplastic selected. These are recommendations provided by the thermoplastic manufacturer. Time and temperature can be changed prior to or during a session by depressing – or + on the home screen. View all factory presets with the horizontal scroll on the home screen with < or >
- **Note:** the wavy white lines indicates that the water is heating up. It will change to green box with > symbol when the set temp is reached and the session can begin.

Home Screen

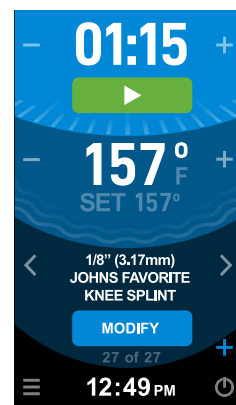

- The menu consists of the following features:
  - Set auto on/off** – this feature automatically sets “on” time and “off” time for specific days of the week. Factory default for this is on. This feature preheats the water to reach set temperature prior to a session starting and to save energy in the evening when not in use.
  - Water evacuation** – when “start” button is pushed, the pump will evacuate the water via the drain hose. Important: be sure that the drain hose is properly inserted in the back of the unit. Drainage can be stopped at any time by pushing the “stop” button. The pump will automatically stop once the water level has sufficiently dropped.
  - Sanitation cycle** – Strava Solutions highly recommends daily sanitation of the splint bath. The sanitation cycle factory default is “on”. The unit is set to engage in a nightly sanitation cycle at 8:00pm (20.00 hrs) Sunday through Thursday. The time and day can be modified by clicking “auto sanitation”. When sanitation cycle is engaged, the unit will heat the water to an extremely high temperature (~ 185°F/85°C) to kill microbes in the water. After the sanitation cycle is completed, the unit will return to last preset used (depending upon unit was set auto on/off).



If sanitation cycle is manually turned on, the 5 minute cycle will run when the “start” button is depressed. The water temperature is displayed on the control panel during the sanitation cycle. At the conclusion of the cycle, the water temperature last used preset temperature.

Only if auto on/off has been set will the unit go into sleep mode after auto sanitation.



**RISK OF SEVERE BURN!**

- Keep the lid closed during sanitation cycle. Do not insert any thermoplastics or any other materials into the bath during sanitation cycle. Do not put hands or appendages in the water.

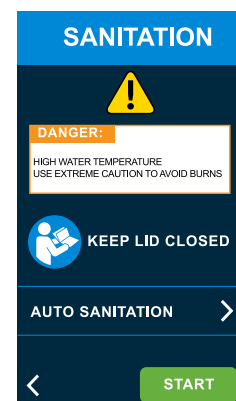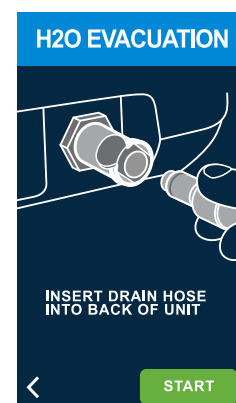

# INSTRUCTIONS CONT.

- Helpful tips – this screen provides the user with helpful tips and information about the Rolyan splint bath
  - Presets – in addition to the factory presets, the user can program desired presets by name. Up to 50 user-defined presets can be stored in the unit. The default time for a new user preset is 1:00 minute and the default temperature is 155°F/68°C.
    - To add a new user preset: 1. go to user presets in the menu, click +, enter the material size (if desired), the sheet name, and adjust the time and/or temperature with – and +. Click save. 2. From the home screen, click the + in the bottom right corner beside the displayed preset. Enter the material size (if desired), the sheet name, and adjust to the desired time and/or temperature with the – and +. Click save.
    - To modify an existing preset: go to user presets in the menu, click on modify, make desired time and/or temperature change with – and +. Click save.
    - **Note:** factory preset names cannot be changed or deleted. User defined presets can be removed.
  - Temp setting – set in degrees Fahrenheit (F) or Celsius (C). Factory default is F.
  - Set time - set the real time clock with scroll wheel in either 12 hour or 24 hour time display. Factory default is 12 hour display mode.
  - Audio/visual – adjust the screen brightness and the volume of auditory signals. A beeping sound engages the last ten seconds of a session to alert the user.
- Note:** audio can be shut off except on certain error message screens.
- Factory reset – **CAUTION!** by clicking reset, all factory defaults will be restored and all user-defined presets will be erased.

New User Preset

– 01:00 +

– 160°F +

ENTER SHEET SIZE

ENTER SPLINT NAME

ENTER SPLINT NAME 2

< SAVE

---

## General Use:

- Once the unit is filled with water, the power is on, the preset is fixed, and the set temperature has been reached, the unit is ready for the thermoplastic materials.
- Insert the splinting material into the reservoir, being careful not to splash hot water outside the tank.
- Press start (green button with arrow on home screen). At any time during a session, the timer can be paused and restarted from the beginning or from the time the unit was paused.
- To maintain an accurate water temperature, retain heat, and minimize evaporation, keep lid closed.
- Use caution when retrieving the material from the bath. Apply the material to the patient as per the splint manufacturer's instruction.
- Maintain sufficient water level at all times. (approx 5"/13cm deep).



CAUTION! WARNING!

**Note:** The water pump and UV light are always on during normal operation of the unit. Mention here the continual use of the pump and uv light during normal operation of the unit

## Emptying the Water:

- Allow the water to cool before water evacuation. Water will not drain unless the water temperature is below 165°F/74°C.
- Be sure that the drain hose is properly inserted at the back the unit. The water will not drain if the hose is not connected.
- In the menu on the control panel, click on H2O Evacuation and press start.
- Once the bath is empty, proceed with tank cleaning.

## Cleaning the bath:

- Rolyan recommends bi-weekly water reservoir cleaning.
- Turn the power switch off and unplug the unit from the wall receptacle. Drain the water.
- Using a soft cloth with mild detergent, wipe out the reservoir. Sanitation wipes (i.e CaviWipes can be used). For hard water spots, use a vinegar and water solution. Rinse and wipe dry.
- Refill with water as per the instructions for filling the tank. (found in initial start up section of the manual)
- **Note:** do not use bleach, diluted bleach or peroxide-based agents in the water bath.

---

## Troubleshooting

Show all error messages, what they look like and how to correct

### Over temp:

If the unit exceeds 193° F/89° C turn off mains power and contact technical service.

### Low water:

1. If there is water in the reservoir, turn off the mains power and contact technical service.
2. If there is no water in the reservoir, turn off the mains power and investigate possible causes - water evaporation or unit leakage.
  - **Water evaporation** - always maintain adequate water volume in the tank.
  - **Water leakage** - turn off mains power and contact technical service.

### UV lamp defective:

Turn mains power off. Unplug cord from unit and wall. Remove rear access panel via 4 screws. Carefully remove black rubber boot from UV housing, allowing the lamp to slide out of the housing. Disconnect lamp from connectors on both ends. Replace bulb. Reconnect at both ends and insert new bulb back into the housing. Attach rear access panel. Dispose of defective bulb according to local regulation.

### Pump occlusion:

Refers to blockage in the water system.

1. If evacuating the water, stop evacuation mode and contact technical service.
2. In standard operation, turn off the mains power and contact technical service.

### Temp sensor error

## Replacement Parts

Heating Element	REF 300.100
UV Lamp	REF 300.105
Mains Power Cord (US Hospital Grade)	REF 300.107
Hose	REF 200.101

---

## Warranty/Replacements

Strava Solutions warrants that its products are free from defects in material or workmanship. Under normal use and following all guidelines defined in this manual, Rolyan splint baths are warranted for a period of one year from when product is received. Should replacement or repair be required, purchaser must notify dealer or manufacturer in writing. After obtaining an RA (returned goods authorization), product must be returned in original packaging.

## Service Life

We estimate a service life of five years for this product, provided it is used in strict accordance with the intended use as set out in this document and all maintenance and service requirements are met. The estimated service life can be exceeded if the product is carefully used and properly maintained, and provided technical and scientific advances do not result in technical limitations. The service life can also be considerably reduced by extreme or incorrect usage. The fact that we estimate a service life for this product does not constitute an additional warranty

## Storage and Handling






- Check the power cord and plug for excessive wear or fraying. Replace as needed.

It is recommended the following guidelines are used whenever this system is being stored or transported another location:

Environment (Temperature)	Operation: 32° F – 104° F (0° C – 40° C)
	Storage: 32° F – 140° F (0° C – 60° C)
Environment (Humidity)	Operation: Up to 80%
	Storage: Up to 90%, non-condensing



## Product Labeling

EC REF	
 <b>STRAVA</b> 2733 Kanasita Drive, Suite 125 Hixson, TN 37343 USA	
Made in USA	
REF 400.100	120V 60HZ ?A
	CE
GTIN	
SN	UL???
 (01)04032766230977(10)0015857098	 



MANUFACTURED BY:

Strava Solutions, LLC

2733 Kanasita Drive, #125 | Hixson, TN 37343 USA

TEL: 1.423.313.6157 | EMAIL: [technicalservice@kismetus.com](mailto:technicalservice@kismetus.com)